

### OVERVIEW

NevadaNano's MPS Methane Gas Sensor provides quick and accurate detection of methane across a variety of industries—from the oil and gas supply chain to safety applications. The smart sensor is intrinsically safe, robust, and extremely poison-resistant. It has built-in environmental compensation and self-testing for fail-safe operation. Sensor readings are output on a standard digital bus or industry-standard analog output – no added electronics are required. With calibration-free operation for 5+ years, the MPS Methane Gas Sensor delivers industry-leading performance and a low cost of ownership.

### PERFORMANCE

Range	500 - 1,500 ppm
Resolution	1 ppm
Calibration	Factory calibrated

### ENVIRONMENTAL OPERATING RANGE

Temperature	-40 to 75 °C
Humidity	0 to 100 %RH
Pressure	80 to 120 kPa



### FEATURES


- Built-in environmental compensation
- Inherently poison-resistant
- No calibration required
- Supports 15+ year lifetimes
- Low power — 29 mW average
- Intrinsically safe (IS) certified
- Built-in self-test for fail-safe operation

### OPERATING PRINCIPLE

The Molecular Property Spectrometer (MPS) Methane Gas Sensor's transducer is a micro-machined membrane with an embedded Joule heater and resistance thermometer. The MEMS transducer is mounted on a PCB and packaged inside a rugged enclosure open to ambient air. Presence of methane causes changes in the thermodynamic properties of the air/gas mixture that are measured by the transducer. Sensor data are processed by patented algorithms to report accurate concentrations.

SPECIFICATIONS ARE SUBJECT TO CHANGE WITHOUT NOTICE.

### MECHANICAL

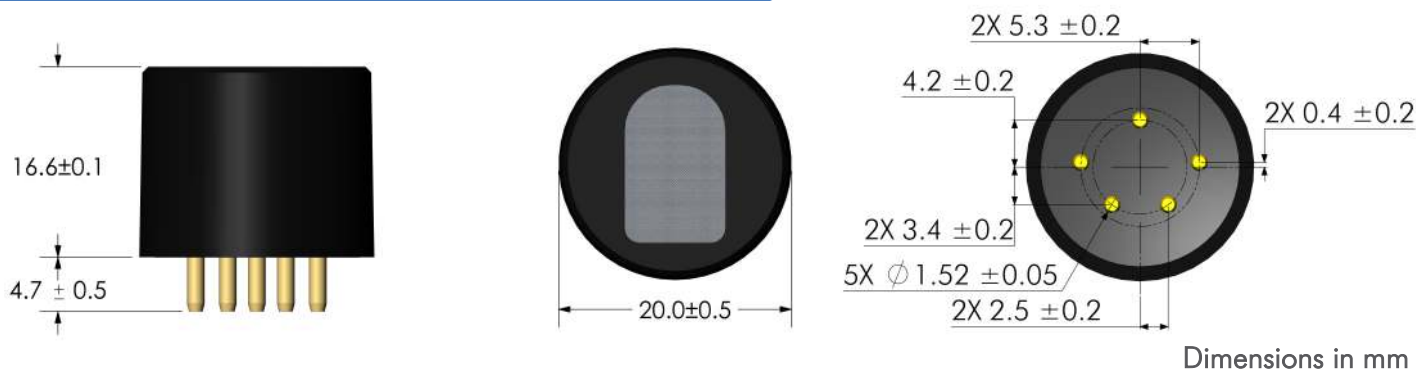

Dimensions 16.6 mm (H) x 20.0 mm (D)

Mass  $8.0 \pm 0.5$  grams


Body material Ultem PEI

### ELECTRICAL

Operating voltage 3.3 - 5.0  $\pm 5\%$  VDC


Current consumption	Average	Operating Range
	8.9 mA	5.0-21.0 mA

5-pin  
Digital Input/Output



Communication: UART  
 Logic signaling standard: 3.3 V  
 Baud rate: 38,400. 8 data, 1 stop bits. No parity  
 RX Data Input : Do not exceed 3.6 V  
 Input High Voltage ( $V_{IH}$ ) = 2.0 V minimum  
 Input Low Voltage ( $V_{IL}$ ) = 0.85 V maximum  
 TX Data Output : Source / Sink 4 mA maximum  
 Output High Voltage ( $V_{OH}$ ) = 2.45 V minimum  
 Output Low Voltage ( $V_{OL}$ ) = 0.45 V maximum  
 Programmable Analog out (optional)

5-pin or 3-pin  
Analog Output



Standard analog output configuration is shown on page 3.  
 Note: "zero" voltage and sensitivity slope can be configurable between 0.04 and 2.9 V, including rising or falling V/ppm.  
 Contact NevadaNano for details.






### SELF-DIAGNOSTICS

The MPS Methane Gas Sensor automatically performs dozens of built-in tests every 2 seconds to ensure fail-safe operation. The MPS alerts the user of any sensor failure or status alert. For additional information on how to interpret and handle detected faults, refer to the MPS Methane Gas Sensor User Manual at:

[www.nevedanano.com/downloads](http://www.nevedanano.com/downloads)

SM-DS-0005-10

### CERTIFICATION

Certification Body				
Test Standard	IEC 60079-0:2017 IEC 60079-11:2011	ATEX NB 2809 UKEX AB 1725 EN 60079-0:2018 EN 60079-11:2012	FM 3600:2018 FM 3610:2018 ANSI/UL 913:2019	CSA 22.2 60079-0:2019 CSA 22.2 60079-11:2014
Protection Categories	Ex ia IIC Ga Ex ia IIIC Da  Ta = -40°C to 75°C	 Ex II 1 G Ex ia IIC Ga  Ex II 1 D Ex ia IIIC Da  Ta = -40°C to 75°C	Class I, Division 1, Group A,B,C,D Class II and III, Division 1, Group E,F,G  Class I, Zone 0 AEx ia IIC Ga Zone 20 AEx ia IIIC Da  Ta = -40°C to 75°C	Class I, Division 1, Group A,B,C,D Class II and III, Division 1, Group E,F,G  Class I, Zone 0 Ex ia IIC Ga Zone 20 Ex ia IIIC Da  Ta = -40°C to 75°C
Certificate	IECEX FMG 19.0028U	FM19ATEX0184U FM21UKEX0159U	FM19US0145U	FM19CA0077U


For additional information on certifications, refer to the MPS Hazardous Locations User Guide here: [www.nevedanano.com/downloads](http://www.nevedanano.com/downloads)

Certificates of Compliance	Specification	Test Lab/Certification Body	Certificate/Report Number
Certificate of Registration of Quality Management System	ISO 9001:2015	National Standards Authority of Ireland (NSAI)	19.8213
IECEX Quality Assessment Report	IEC 80079-34:2018	FM Approvals LLC	GB/FME/QAR19.0020/00
ATEX Quality Assurance Notification	2014/34/EU	FM Approvals LLC	FM19ATEXQ0200
UK Quality Assurance Notification	UKSI 2016:1107 (as amended)	FM Approvals LLC	FM21UKQAN0168
RoHS (2 & 3) Compliant	2011/65/EU & 2015/863	Underwriters Laboratories	CETR-NNT01.1
China RoHS Compliant	SJT/T 11363 & 11364	Underwriters Laboratories	CETR-NNT01.1
REACH Compliant	EC 1907/2006 (33 & 67)	Underwriters Laboratories	CETR-NNT01.1

The certificates of compliance are available at [www.nevedanano.com/downloads](http://www.nevedanano.com/downloads)

### ANALOG OUTPUT CONFIGURATION

The plot below shows the standard analog output configuration of the MPS Methane Gas Sensor.

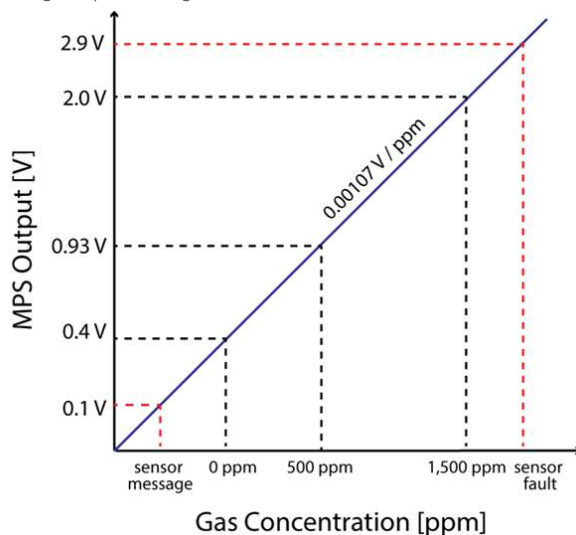

SM-DS-0005-10

### ADDITIONAL TEST STANDARDS

Test	Specification	Summary of Test Conditions
Low Temperature Operating	IEC 60068-2-1	500 Hours @ -50°C
High Temperature Operating	IEC 60068-2-2	1000 Hours @ 85°C
Vibration	IEC 60068-2-6	31Hz – 150 Hz (2G acceleration), 1 hour per axis, 3 axes
Shock	IEC 60068-2-27	50G peak/11ms half sine pulse, 3 axes (positive and negative pulses)
Drop	IEC 60068-2-31	1-meter drop onto concrete
Damp heat - steady state	IEC 60068-2-78	500 hours @ 40°C/93% RH
Temperature cycling	JESD22-A104E	From -40°C to 85°C for 200 cycles
Sand/Dust	MIL-STD-810G Method 510.5	Sand: 150-850 $\mu\text{m}$ SiO <sub>2</sub> particle size, 23 m/s nom. velocity, 1.5 hrs @ 70°C per axis, 3 axes Dust: Red China Clay, 1.5 m/s nom. velocity, 6 hrs @ 20°C and 6 hrs @ 70°C
Poisoning	NevadaNano	1,200 ppm-hours H <sub>2</sub> S (50 ppm for 24 hours) 10,400 ppm-hours siloxanes (Decamethylcyclopentasiloxane) (100 ppm for 4 hours, then 1,000 ppm for 10 hours) 0.25 ppm-hours NO <sub>2</sub> (3 ppm for 5 minutes) 0.83 ppm-hours HCN (10 ppm for 5 minutes) 0.75 ppm-hours SO <sub>2</sub> (9 ppm for 5 minutes) 0.17 ppm-hours Cl <sub>2</sub> (2 ppm for 5 minutes) 4.17 ppm-hours NH <sub>3</sub> (50 ppm for 5 minutes)
Electrostatic Discharge	JEDEC JS001-2017	Human Body Model, passed at 2 kV
EMC: Radiated Emissions	EN 55011	30 MHz to 1 GHz
EMC: RF Electromagnetic Field Immunity	IEC/EN 61000-4-3	80 MHz to 6 GHz at 10 V/m
EMC: Magnetic Immunity	IEC/EN 61000-4-8	30 A/m, 3 axes, 50 Hz and 60 Hz

The table above provides a summary of standardized tests and test conditions to which the MPS Extended Range Methane Gas Sensor has been subjected. The sensor has passed all of these tests by demonstrating normal gas detection performance both before and after each test.

### PART NUMBER ORDERING GUIDE

Please refer to the following table below when ordering the MPS Methane Gas Sensor. When ordering a MPS S4 Evaluation Kit, please specify the MPS Methane Gas Sensor part number to be evaluated.



Manufacturer Part Number	Description
MPS005-S40505-EX	MPS Methane Gas Sensor, S4, 5-Pin, UART + Analog Out + Auto
MPS005-S40509-EX	MPS Methane Gas Sensor, S4, 5-Pin, UART + Analog Out + Auto Start
MPS005-S40309-EX	MPS Methane Gas Sensor, S4, 3-Pin, Analog Out + Auto Start



Manufacturer Part Number	Description
MPS999-S40000-99	MPS S4 Evaluation Kit



Nevada Nanotech Systems Inc.  
 1395 Greg Street, Suite 102  
 Sparks, Nevada 89431  
 United States  
 Tel: +1 775 972 8943  
 Fax: +1 775 972 8078  
[info@nevedanano.com](mailto:info@nevedanano.com)  
[www.nevedanano.com](http://www.nevedanano.com)

SPECIFICATIONS ARE SUBJECT TO CHANGE WITHOUT NOTICE.

SM-DS-0005-10